

**NOISE POWER SPECTRUM OF COMPUTED MAMMOGRAPHY AND
FULL FIELD DIGITAL MAMMOGRAPHY**

FAEZEAH BINTI ABD GHANI

UNIVERSITI TEKNOLOGI MALAYSIA

NOISE POWER SPECTRUM OF COMPUTED MAMMOGRAPHY AND FULL
FIELD DIGITAL MAMMOGRAPHY

FAEZEAH BINTI ABD. GHANI

A dissertation submitted in fulfilment of the requirement for the award of the degree
of Master of Science (Physics)

Faculty of Science
Universiti Teknologi Malaysia

JANUARY 2014

To my beloved ibu, ayah and my

Lovely siblings

ACKNOWLEDGEMENT

In the name of ALLAH, the most merciful and beneficial

I would like to express my deepest gratitude and heartfelt thanks to everyone who assisted me in the completion of this dissertation. In particular, I would like to give a special thanks to Assoc. Prof. Dr. Wan Muhamad Saridan Wan Hassan for his supervision, guidance, advice and support that has enabled me to develop an understanding of the subject. I am indebted to him more than he knows.

I would also like to thank all the staff of Hospital Sultan Ismail, Hospital Enche' Besar Hajjah Kalsom, Kluang and Malaysian Institute of Nuclear Technology, MINT with whom I had pleasure of working with. I would also like to dedicate thanks to all the staff of Universiti Teknologi Malaysia, UTM especially Physics Department library and Perpustakaan Sultanah Zanariah library for all the book and references provided. I would also like to thanks Malaysia government for give me financial support along my studies in UTM through MyBrain15 programme.

Words fail me to express my appreciation to my beloved family especially to my mother, Manis Bte Othman and my father, Abd Ghani Bin Pendek whose dedication, love and persistent confidence in me have taken the load off my shoulders. A big hug to my lovely siblings for the continuous supporting me in completing this dissertation. Finally, lots of thanks to all my friends who are with me from the beginning till the end. Thank you all.

ABSTRACT

Noise in medical imaging is one of the parameters that need to be measured in image analysis. Noise of an image can be measured by noise power spectrum (NPS). A comparison of two types of mammography imaging machine namely Hologic Lorad Selenia Full-field Digital Mammography (FFDM) and Hologic Lorad M-IV Series Computed Mammography (CM) has been made to identify the system of mammography that has higher noise level. Both types of machine use automatic exposure control (AEC) for image acquisition. A potential of 30 kVp and 110 mAs-120 mAs has been applied. The images that are obtained from both of machines are analysed using MATLAB programme MATLAB Version 7.8.0 (R2009a). The best technique of NPS computations, Dobbin's method has been applied. NPS is shown using 2-Dimensional mesh plot and 1-Dimensional graph taken from the extraction of 2-Dimensional graph where the noise power spectra versus values spatial frequency are shown. Noise level of the images from both machines are studied and compared. The sensitivity of NPS is at lower spatial frequency. The comparison shows that at lower spatial frequency, CM image has higher noise level compared to FFDM image, and at higher frequency, FFDM image has higher noise level compared to CM image. The noise level is in the range of 10^{-3} - 10^{-6} mm². In conclusion, CM has higher noise compared to FFDM.

ABSTRAK

Hingar dalam pengimejan perubatan merupakan salah satu parameter yang perlu diukur dalam menentukan kualiti sesuatu imej. Hingar imej boleh dikira melalui spektrum kuasa hingar. Perbandingan antara dua jenis mesin mammografi iaitu Hologic Lorad Selenia Full-field Digital Mammography (FFDM) dan Hologic Lorad M-IV Series Computed Mammography (CM) dilakukan untuk menentukan mesin mammografi yang mempunyai hingar yang lebih tinggi. Kedua-dua jenis mesin menggunakan pengawalan dedahan automatik (AEC) untuk penghasilan imej. Dedahan sebanyak 30 kVp dan 110-120 mAs digunakan. Imej yang terhasil daripada kedua-dua jenis mesin dianalisis menggunakan program MATLAB, MATLAB Versi 7.8.0 (R2009a). Teknik terbaik untuk mengira spektrum kuasa hingar adalah menggunakan kaedah Dobbin. Spektrum kuasa hingar dipaparkan menggunakan graf 2-Dimensi dan graf 1-Dimensi diperolehi melalui hirisan graf 2-Dimensi dimana spektra kuasa hingar melawan frekuensi ruang. Spektrum kuasa hingar untuk kedua-dua jenis mesin dianalisis dan dibandingkan. Sensitiviti pengiraan spectrum kuasa hingar terletak pada frekuensi ruang yang rendah. Perbandingan menunjukkan pada frekuensi ruang yang rendah, imej CM mempunyai nilai hingar yang tinggi, dan pada frekuensi ruang yang tinggi, imej FFDM yang mempunyai nilai hingar yang lebih tinggi. Nilai hingar yang diperolehi terletak antara julat 10^{-3} - 10^{-6} mm². Kesimpulannya, imej CM mempunyai nilai hingar yang lebih tinggi daripada imej FFDM.

TABLE OF CONTENTS

CHAPTER	TITLE	PAGE
	DECLARATION	ii
	DEDICATION	iii
	ACKNOWLEDGEMENT	iv
	ABSTRACT	v
	ABSTRAK	vi
	TABLE OF CONTENTS	vii
	LIST OF TABLES	x
	LIST OF FIGURES	xii
	LIST OF SYMBOLS AND ABBREVIATIONS	xv
	LIST OF APPENDICES	xvii
1	INTRODUCTION	1
	1.1 Background of Study	1
	1.1.1 Analogue Mammography System	2
	1.1.2 Digital Mammography System	3
	1.2 Statements of Problem	5
	1.3 Objectives of Study	5
	1.4 Limitation of Study	6
	1.5 Significance of Study	6

1.6 Thesis Outline	7
2 LITERATURE REVIEW	8
2.1 Computed Mammography	8
2.2 Full Field Digital Mammography	12
2.3 Physical Image Quality	13
2.4 Noise	16
2.4.1 Quantum Noise	16
2.5 Fourier Transform	17
2.6 Noise Power Spectrum	18
2.7 Spatial Frequency	20
3 RESEARCH METHODOLOGY	21
3.1 Introduction	21
3.2 Image Preparation	22
3.2.1 Perspex Preparation	23
3.2.2 Image Acquisition for FFDM	23
3.2.3 Image Acquisition for CM	25
3.2.3.1 Digitization of Film	28
3.2.4 Image Dataset	28
3.3 Computer Programming	29
3.4 NPS Computation Method	30
3.4.1 Dobbin's Method	30
4 RESULTS AND DISCUSSION	32
4.1 Introduction	32
4.2 NPS for FFDM Images	32

4.2.1	Effect of Fourier Length FFT	35
4.2.2	Comparison of Curve	38
4.3	NPS for CM Images	41
4.3.1	Effect of Fourier Length FFT	44
4.3.2	Comparison of Curve	46
4.4	Comparison of NPS on CM and FFDM	50
5	CONCLUSION AND FUTURE WORK	54
5.1	Conclusions	54
5.2	Future Work	55
	REFERENCES	56
	APPENDIX	59

LIST OF TABLES

TABLE NO.	TITLE	PAGE
3.1	Detailed information of the images used in this research.	29
4.1	NPS values at low spatial frequency, 0 – 1 cycle/mm for ffdm1 image.	36
4.2	NPS values at low spatial frequency, 0 – 1 cycle/mm for ffdm2 image.	37
4.3	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 64	39
4.4	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 128	40
4.5	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 256	41
4.6	NPS values at low spatial frequency, 0 – 1 cycle/mm for cm1 image	45
4.7	NPS values at low spatial frequency, 0 – 1 cycle/mm for cm2 image	46
4.8	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 64.	47
4.9	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 128	48
4.10	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 256	49

4.11	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 64	51
4.12	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 128	52
4.13	NPS values at low spatial frequency, 0 – 1 cycle/mm at L = 256	53

LIST OF FIGURES

FIGURE NO.	TITLE	PAGE
1.1	The Hurted & Driffield (H&D) curve describes optical density (OD) vs. the logarithms (base 10) of exposure	3
2.1	Exposed imaging plate is scanned by laser while being conveyed. Light emission created is detected by PMT.	10
2.2	Imaging Plate Luminescence Mechanism. (a) Band structure representation of a bound electron-hole pair or exciton. (b) The energy levels at which an electron-hole can be trapped at a PSL complex	10
2.3	The characteristics response of screen-film and computed radiography photostimulabe phosphor detector	11
2.4	Mechanism for FFDM	12
2.5	Breast radiography	15
3.1	Flow chart of research methodology	22
3.2	6 pieces of Perspex as phantom	23
3.3	Hologic Lorad Selenia Full Field Digital Mammography available at Diagnostic Imaging Department, Hospital Sultan Ismail, Johor Bahru	24
3.4	Mammographic phantom (Perspex) located on the grid of the machine	24
3.5	Hologic Lorad M-IV Series Screen-Film Mammography available at Diagnostic Imaging Department, Hospital Eche'	25

Besar Hajjah Kalsom, Kluang

3.6	C-PLATE Series used for mammography	26
3.7	Direct Digitizer REGIUS MODEL 210 Computed Radiography	26
3.8	DRYPRO MODEL 873 Laser Imager	27
3.9	Films that being produced for CM	27
3.10	DR 3000HD Digital Radiograph Film Digitisation System available at MINT	28
3.11	Block diagram describing steps to compute NPS	30
3.12	Flow chart describing steps to compute NPS by Dobbin's method	31
4.1	2-Dimensional NPS for ffdm image.	33
4.2	1-Dimensional slice extraction graph for ffdm.	34
4.3	NPS for different of L for ffdm1.	35
4.4	NPS for different of L for ffdm2.	37
4.5	NPS curve for ffdm1 and ffdm2 at L=64	38
4.6	NPS curve for ffdm1 and ffdm2 at L=128	39
4.7	NPS curve for ffdm1 and ffdm2 at L=256.	40
4.8	2-Dimensional NPS for cm image.	42
4.9	1-Dimensional slice extraction graph for cm.	43
4.10	NPS values for different used of FFT length for cm1.	44
4.11	NPS values for different used of FFT length for cm2.	45
4.12	NPS curve for cm1 and cm2 at L=64	47
4.13	NPS curve for cm1 and cm2 at L=128.	48
4.14	NPS curve for cm1 and cm2 at L=256	49

4.15	NPS for FFDM and CM images at L=64	50
4.16	NPS for FFDM and CM images at L=128	51
4.17	NPS for FFDM and CM images at L=256	52

LIST OF SYMBOLS AND ABBREVIATIONS

I	-	Intensity with film
I_0	-	Intensity without film
\bar{I}	-	Average background intensity
(x, y)	-	Spatial coordinates
(u, v)	-	Spatial frequency coordinates
$\Delta_x \Delta_y$	-	Pixel sizes in x and y axis
L	-	Length of FFT
N_x, N_y	-	Number of element
$\Delta D(x, y)$	-	Radiographic fluctuating components
BaFBr	-	Barium fluorobromide
BaFI	-	Barium flourohalide
Eu	-	Europium
a-Se	-	amorphous selenium
CaI	-	Caesium Iodide
ADC	-	Analogue Digital Converter
OD	-	Optical Density
CCD	-	Charged Couple Detector
CR	-	Computed Radiography
FFT	-	Fast Fourier Transform

NPS	-	Noise Power Spectrum
NNPS	-	Normalized Noise Power Spectrum
NQE	-	Noise Equivalent Quanta
MTF	-	Modulation Transfer Function
DQE	-	Detective Quantum Efficiency
CM	-	Computed Mammography
FFDM	-	Full-Field Digital Mammography
T	-	Transmittance
PSP	-	Photostimulable Phosphors Detector
PSL	-	Photostimulated Luminescence
PMT	-	Photo Multiplier Tube
TFT	-	Thin Film Transistor
QA	-	Quality Analysis
WS	-	Wiener Spectrum
ROI	-	Region of Interest
SNR	-	Signal Noise Ratio
TORMAM	-	Test Object Mammography
CDMAM	-	Contrast-detail Mammography

LIST OF APPENDICES

APPENDIX	TITLE	PAGE
A	MATLAB Programme to Compute NPS	59

CHAPTER 1

INTRODUCTION

1.1 Background of Study

Breast cancer is the most common cancer among women. In 2007, it is recorded in Malaysia breast cancer contributes 32.1 % meanwhile the other 67.9 % is for other cancers (Omar and Ibrahim, 2011). Technology developments in radiographic imaging insist clinicians in order to cure the cancer hence to reduce this percentage. Radiographic imaging specially mammography is used to detect the existence of breast cancer. The first mammography that was invented is film-screen mammography followed by computed mammography and full field digital mammography for current technologies.

Development of technology in medical fields especially in medical imaging field aids in image analysis. Digital system shows many advantages compared to analogue system. This includes low spatial resolution, higher contrast resolution and post processing techniques confer much improved image quality. Other than that, digital mammography also erases the use of film storage. In spite of that, there are some technical differences between digital and analogue that affect the reader's analysis of lesion (Gay *et al.*, 2010).

1.1.1 Analogue Mammography System

Analogue system also known as conventional screen film system. This system is the pioneer system for recent radiography system (digital). This system has high resolution, simple, established, large areas and cheap. However, this system has limited dynamic range, need post-processing, and low speed. Basically, this system needs the usage of film. Composition of film usually, tabular grain emulsion, cubic grain emulsion and film emulsion which is silver halides (AgBr and AgI). It is bonded in a gelatine base. After exposure, latent image will be formed, which altered chemical bond. During film processing, latent image is visible by chemical reduction of the silver halides into metallic silver grains.

The image formed by film or in the form of a TV voltage, makes it harder to analyse the image. Subjective or semi-quantitative test objects are needed to analyse the image hence assess the image quality. Test object mammography (TOR MAM) and contrast-detail mammography (CDMAM) 3.4 (c-d) test objects are commonly test objects that are used. Test objects help in controlled input signal when imaged under standard conditions and observer needs to analyse the image. Objective image quality was measured by noise power spectrum (NPS) and modulation transfer function (MTF) (Marshall, 2006).

The parameter being measured for screen film radiography is the optical density (OD) of the film. OD is the degree of darkness measured by densitometer. As the exposure high, the film becomes darker. Transmittance (T) depends on the intensity of exposure.

$$T = \frac{I}{I_0} \quad 1.1$$

$$OD = -\log(T) \quad 1.2$$

where, I : Intensity with film

I_0 : Intensity without film

Equation 1.1 shows relationship between intensity with film existence and transmittance. Equation 1.2 indicates that as transmittance increases, the OD decreases. If light totally transmitted, it has 0 OD. If OD is 4, meaning that no light transmit through film. Typical range OD of film for base density and fog density could exceeded of 0.25. Figure 1.1 indicates graph of X-ray exposure that has nonlinear (sigmoid) relationship with optical density of film known as The Hurted & Driffield (H&D) Curve (Testagrossa *et al.*, 2012).

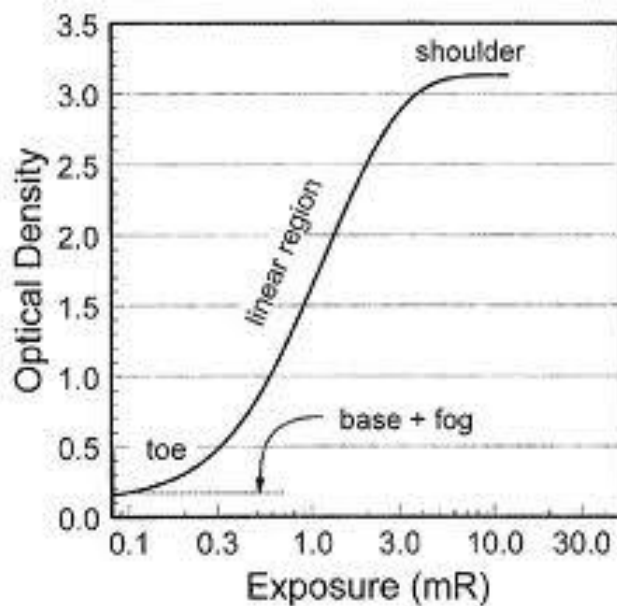


Figure 1.1: The Hurted & Driffield (H&D) curve describes optical density (OD) vs. the logarithms (base 10) of exposure (Testagrossa *et al.*, 2012).

1.1.2 Digital Mammography System

Digital radiography system generally is higher resolution pixel detector than analogue radiography system. Digital radiography uses a digital signal processing. Fully digital mammography consists of direct and indirect conversion radiography system. Indirect conversion consists of image plated based on photostimulable phosphors detector known as computed radiography system (CR) and charged couple detector (CCD). Direct conversion consists of flat panels with amorphous Selenium or Caesium Iodide on amorphous Silicon detector known as full field digital mammography system (FFDM) and semiconductor pixel detector (MedipixI). CCD, CR and FFDM are based on integral read-out architecture; do not allow an effective noise rejection hence, detection contrasts become low of the signal while MedipixI operates in single photon counting mode that has high contrast detection (Bisogni *et al.*, 2005).

CR system possesses half analogue and half digital system. CR uses film cassette and produces latent image (analogue picture). Signals produced in each pixel are analogue packet of charges (ADC) analogue to digital converter during image readout. Computed radiography is used as general digital radiography for applications that require moderate productivity, resolution and dose performance. However, because of some technical limitations, CR system could not produce the resolution performance of the state-of-the-art flat panel image receptor used in full-field digital mammography, FFDM (Smith, 2006).

Basically, amorphous selenium (a-Se) full field digital mammography system functions as breast assessment rather than screening. This system consists two distinct categories which are CR approach and integrated detector. CR involves the use of photostimulable phosphor plates held in cassette. Integrated detector uses an X-ray converter bonded to a thin film transistor (TFT) array which performs the image readout. Image is available directly on the hospital information network for integrated detector compared to CR which is manually handling (Marshall 2006).

1.2 Statements of Problem

Existence of noise produces low quality image, hence resulting a complex image, complicated for the radiologist to analyze. The performance of mammography is being compared in terms of noise. Noise can be quantitatively measured using NPS. The mammography machine with higher NPS is considered as low quality of mammography system. Although, there are some other quality measurements that need to be considered, this study mainly focus on NPS.

1.3 Objectives of Study

The general objective of this study is to identify the mammography system with higher NPS.

The specific objectives are:

- 1) To study and to analyze technique used to evaluate NPS.
- 2) To evaluate noise properties of two mammography systems by using Fast Fourier Transform (FFT) analysis of noise images.

1.4 Limitation of Study

This research is only focus on noise properties. Other physical properties such as spatial resolution and contrast could be analysed to conclude the efficiency of mammography thus, increase the image quality produced.

1.5 Significance of Study

It is important to know the noise power spectrum of mammography system. The information can be used to analyze the efficiency of the type of mammography itself. Hence, further research could be done to calculate the other physical properties, MTF of mammography thus, identify the source problem to improve the efficiency of the mammography machine. These parameters NPS and MTF are also part of the commissioning and routine quality analysis (QA) measurement in European Reference Organisation for Quality Assured Breast Screening and Diagnostic Services (EUREF) Digital Addendum, 2003 (Marshall 2006).

1.6 Thesis Outline

This thesis comprised of 5 chapters. Chapter 1 contains introduction and background of this thesis. Chapter 2 includes literature review that related to this thesis. Chapter 3 explains on how this research being done by using MATLAB programme to get NPS. Chapter 4 shows the results and discussion being made. Conclusion for this thesis and future work are expressed in Chapter 5.

REFERENCES

- Bisogni, M. G. Bulajic, D. Delogu, P. Fantacci, M. E. Novelli, M. Quattrrocchi, M. Rosso, V. Stefanini A. (2005). Performances of Different Digital Mammography Imaging Systems: Evaluation and Comparison. *Nuclear Instruments and Methods in Physics Research: Elsevier A* 546 [14-18]
- Chen, L. Abbey, C.K. and Boone, J. M. (2013). Association between Power Law Coefficients of Anatomical Noise Power Spectrum and Lesion Detectability in Breast Imaging Modalities *Physics in Medicine and Biology*. 58 [1663-1681]
- Dainty, J.C. and Shaw, R. (1974). *Image Science*. London: Academic Press.
- Dobbins III, J. T., Ergun, D. L., Rutz, L., Hinshaw, D. A., Blume, H. And Clark, D. C. (1995) DQE (f) of four generations of computed radiography acquisition devices. *Medical Physics*. 22: [1581-1593]
- Dobbins III, J. T. (2000). Image quality metrics for digital systems. In J. Beutel, H. L. Kundel and R. L. V. Metter (Eds), *Handbook of Medical Imaging* (Vol. 1, pp. 161-222). Bellingham: SPEI Pubs.
- Dobbins III, J. T., Samei, E., Ranger, N. T., and Chen, Y. (2006). Intercomparison of methods for image quality characterization. II. Noise power spectrum. *Medical Physics*, 33(5), [1466-1475]
- Gay, H. Pietrosanu, R. George, S. Tsiaz, D. Mehta, R. Patel, C. Heller, S. Wilkinson, L. (2010). Comparison between Analogue and Digital Mammography, A

Reader's Perspective. Department of Radiology, *St Georges Healthcare NHS Trust*, London.

Hanson, K. M. Newton, T. H. Potts, D. G. (1981) Noise and contrast discrimination in computed tomography. *The Mosby C. V. Company*. London.

Hendee, W. R. and Ritour, R. E. (2002). Medical Imaging Physics. (4th ed.) *Wiley-Liss Publications*. New York.

ICRU (1986) Modulation Transfer Function of Screen-Film System, ICRU Report 41, International Commission on Radiation Units and Measurements. Maryland.

Khairul Anuar B. Mohd Salleh (2009), Evaluation of Imaging Performance of Industrial Digital Radiography Detector System, MSc. Thesis, Universiti Teknologi Malaysia (UTM)

Marshall, N .W. (2006), A Comparison between Objective and Subjective Image Quality Measurements for a Full Field Digital Mammography System, *Physics in Medicine and Biology*. **51** [2441-2461]

Mohammad Hassan Khanmirzaei. (2010), Computation of Detective Quantum Efficiency of Medical X-ray Radiographic Screen-Films, MSc. Thesis Universiti Teknologi Malaysia.

Omar, Z. A. and Ibrahim, N. S. (2011). National Cancer Registry Report: Malaysia Cancer Statistics – Data and Figures 2007, *National Cancer Registry, Ministry of Health Malaysia*: Putrajaya

Penelope, R. and Williams, J. (2008), Farr's Physics for Medical Imaging 2nd Edition, *Saunders Elsevier*. United Kingdom.

Rowlands, J. A. (2002) The Physics of Computed Radiography. *Physics in Medicine and Biology*. 47 [123-166]

- Smith, A.P. (2006) Image Quality of CR Mammography, *Hologic, Inc.* Bedford.
- Smith, A. P (2005) Fundamentals of Digital Mammography: Physics, Technology and Practical Considerations. *Hologic, Inc*, Bedford.
- Testagrossa, B. Acri, G. Causa, F. Novario, R. Tripepi, M. G. Vermiglio, G. (2012) Unified Procedure for Quality Controls in Analogue and Digital Mammography. *InTech Corporation*, Messina.
- Williams, M. B. Elizabeth, A. Krupinski, Keith, J. Strauss, William, K. Breeden, III. Rzeszotarski, M. S. Applegate, K. Wyatt, M. Bjork, S. Seibert, J. A. (2007) Digital Radiography Image Quality: Image Acquisition, *American College Radiology* 4 [371-388]
- Williams, M. B. Mangioficio, P. A and Simoni, P.U. (1999). Noise Power Spectra of Images from Digital Mammography Detectors. *Medical Physics*. 26(7) [1279-1293]
- Zeki Ahmed Darwish (2011), Comparison of the Noise Power Spectrum Properties of Medical Imaging Systems, MSc. Thesis, Universiti Teknologi Malaysia

26 October 2004 DQE evaluation of a full-field digital mammography system. Hans Roehrig; Kunal Gandhi; Jiahua Fan; Ananth Poola; Seiichi Mimura. Author Affiliations +. Physical characteristics necessary to calculate the Detective Quantum Efficiency of a clinically used flat panel imager for full-breast digital mammography are presented. Objective quantities such as modulation transfer function (MTF), noise power spectrum (NPS) and detective quantum efficiency (DQE) have been evaluated. The X-ray photon fluence was determined using Half-Value-Layer (HVL) techniques.